



Measurement of iohexol from canine plasma: comparative analysis between enzyme-linked immunosorbent assay, neutron activation analysis, and high performance liquid chromatography



Victoria Ortín Piqueras¹, Thomas Spillmann², Merja Pöytä Kangas³, Juhana M. Honkavaara², Satu Sankari², Dennis E. Vaccaro⁴, Rafael Frías¹

¹Central Animal Laboratory, University of Turku, Finland

²Department of Equine and Small Animal Medicine, Faculty of Veterinary Medicine, Helsinki, Finland

³Department of Production Animal Medicine, Faculty of Veterinary Medicine, Helsinki, Finland

⁴BioPhysics Assay Laboratory, Inc., Worcester, MA, USA

Introduction

Iohexol (Omnipaque®) is a non-radioactive, iodinated, water-soluble radiographic contrast medium, that is widely used for **imaging purposes** in both the clinical, and research settings. This well known X-ray contrast medium is extensively used worldwide, considered as a secure, economical, and easily available.

This contrast agent is also commonly used as a marker for **glomerular filtration rate** in both humans and animals such as dogs and cats. It has also been used to test **intestinal permeability** in humans, dogs, horses and rats.

Aim of study

To determine the **FIT-GFR Iohexol (ELISA) Kit** accuracy for the measurement of iohexol in canine plasma, and to compare it to both **high-performance liquid chromatography (HPLC)** and **neutron activation analysis (NAA)**.

Materials and Methods

Blank and iohexol-containing plasma samples (n=100) from dogs were collected from the jugular vein in lithium heparin tubes before and after intravenous application of 3.0 g iohexol/dog to the cephalic vein of healthy dogs.

CONCLUSIONS

- ✓ Findings from our study establish that **measurement of iohexol from canine plasma using the ELISA Kit is as reproducible and precise as using HPLC or NAA.**
- ✓ Moreover, using **ELISA Kit** for measuring iohexol may be more practical, economical and useful than using HPLC or NAA.

Results

The results of this study showed that the correlation coefficients when comparing **ELISA vs. HPLC** (r=0.98), **ELISA vs. NAA** (r=0.99) and **HPLC vs. NAA** (r=0.98) were all excellent.

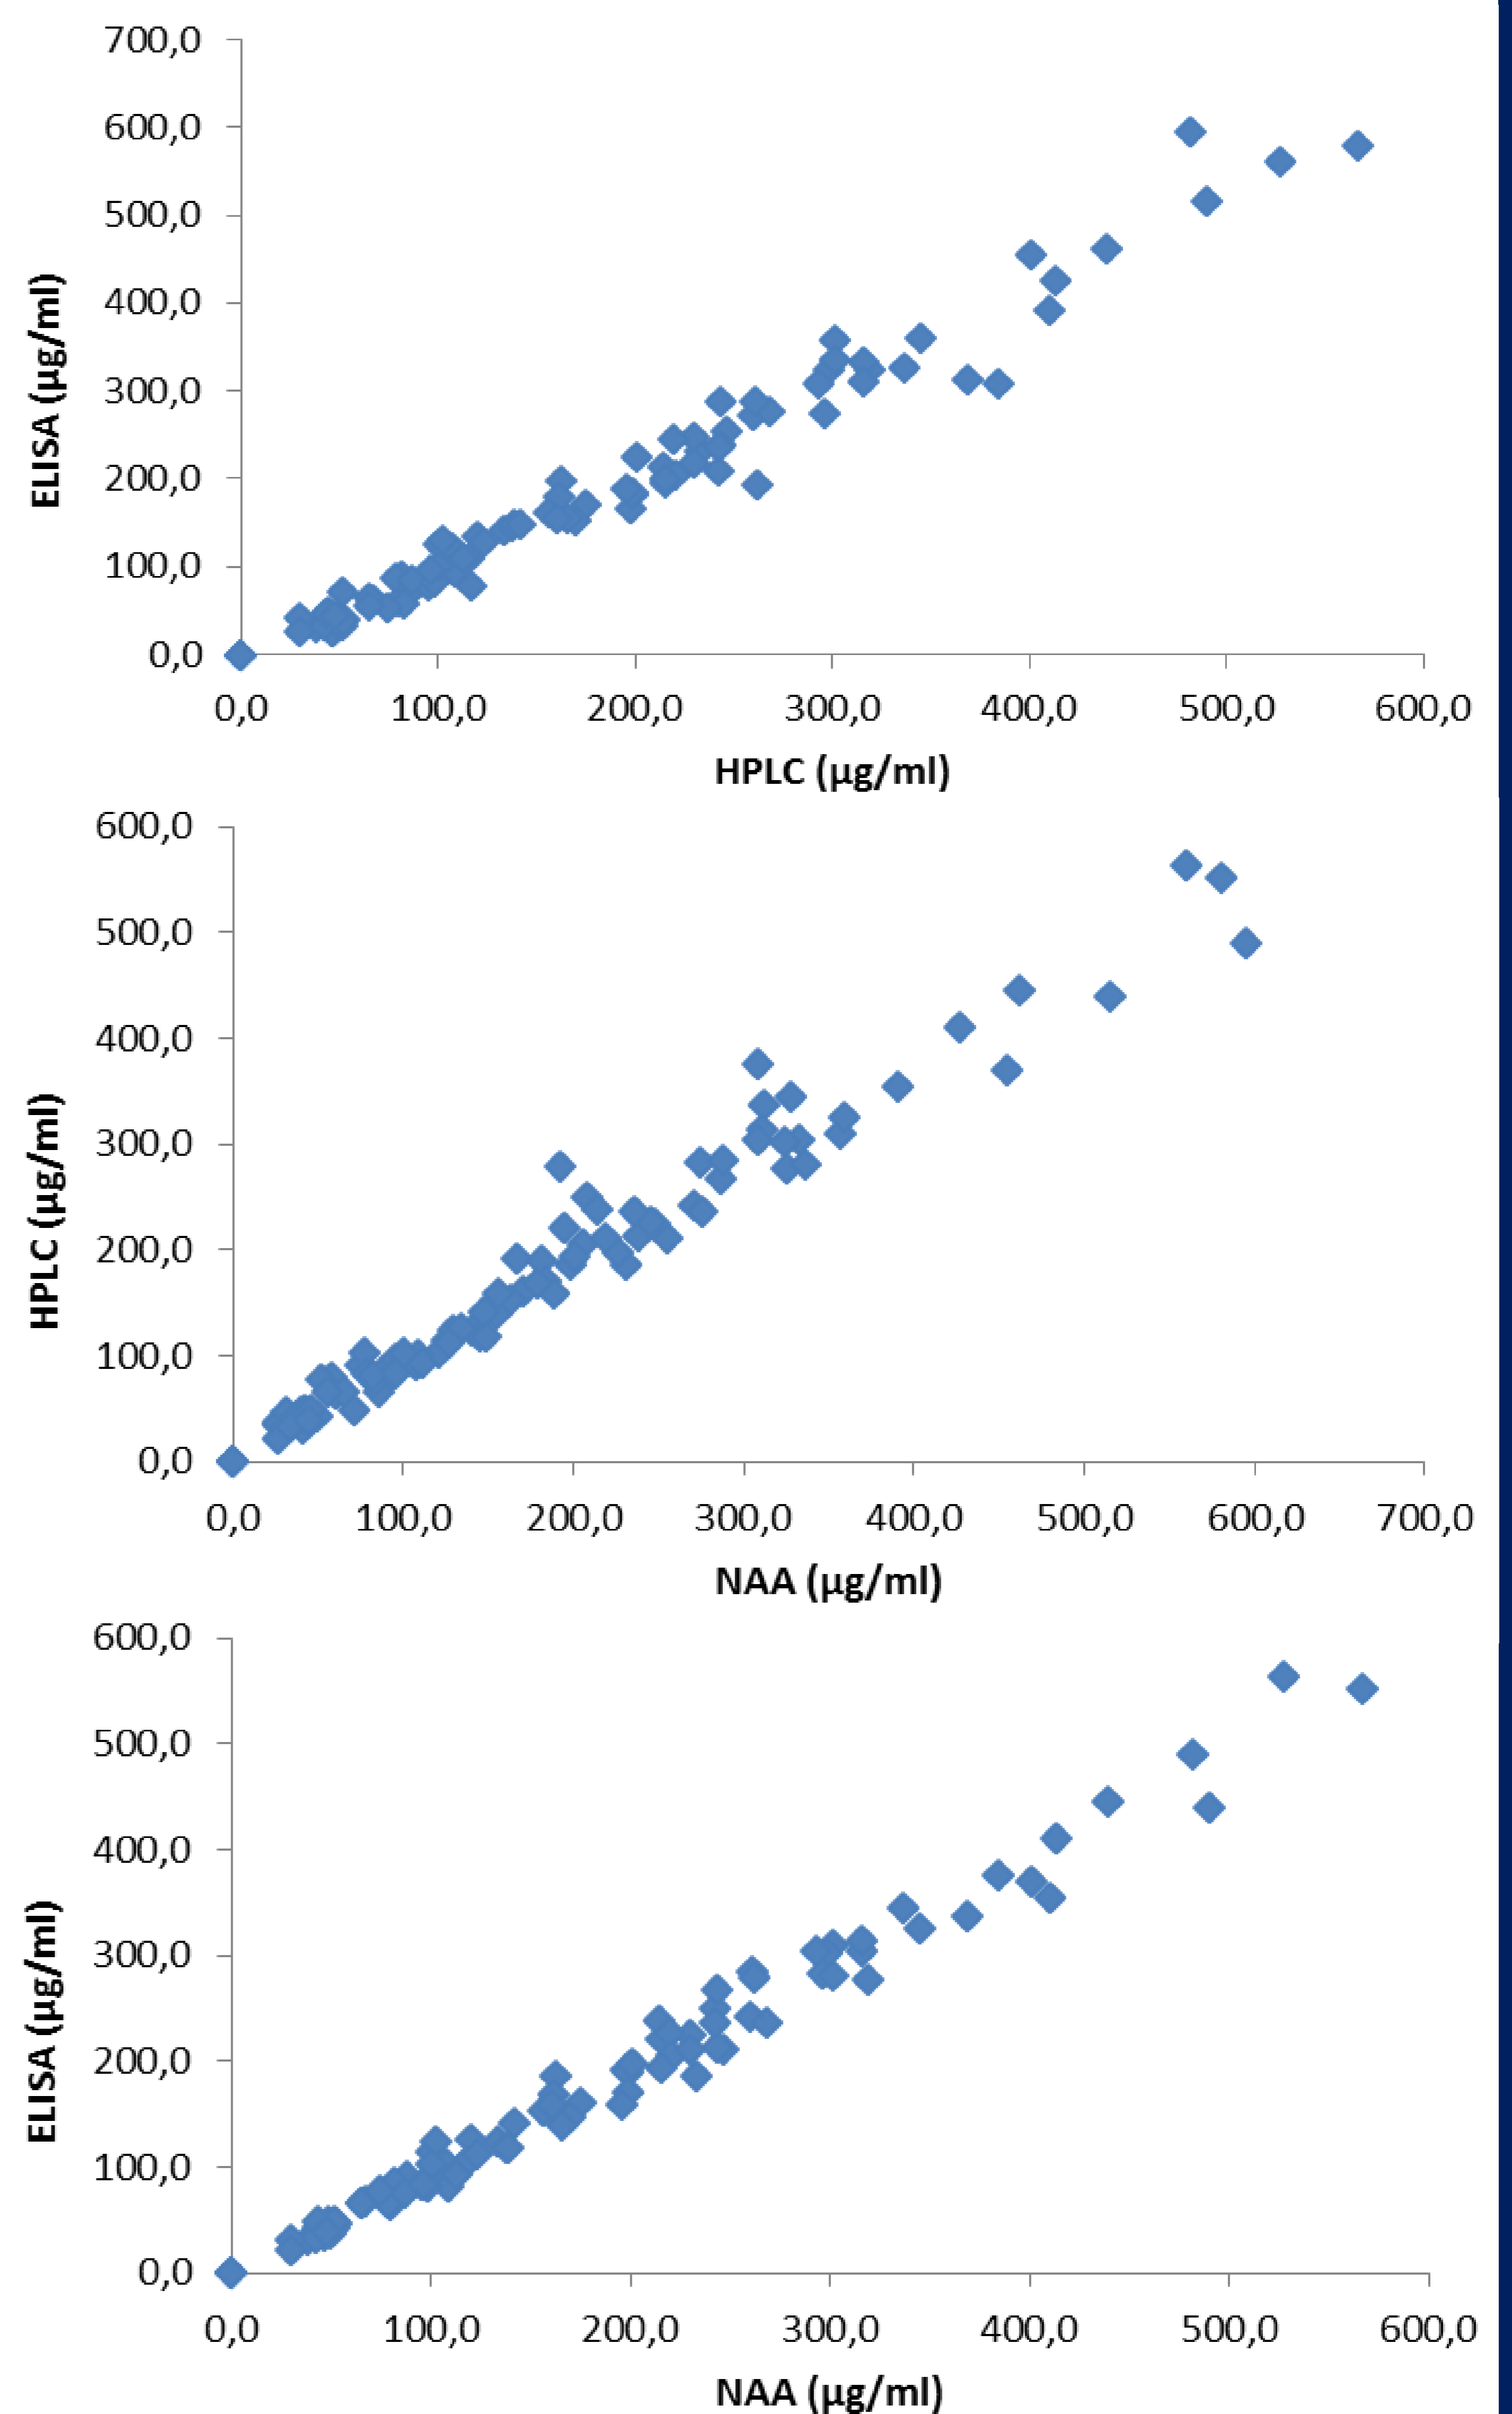


Fig. The iohexol concentration (µg/ml) in collected canine plasma samples measured by ELISA, NAA and HPLC.

Acknowledgements

Financially supported by the Finnish Veterinary Foundation.

References

- [1] Albert DA *et al* (2003). Neutron-activation analysis: A novel method for the assay of iohexol. *J Lab Clin Med*;141:106-9..
- [2] Mandelbrot DA *et al* (2007). Validation of neutron activation as a novel method to determine glomerular filtration rate. *Nephron Clin Prat* 107:C117-122.
- [3] Reinhardt CP *et al* (2001). Stable labeled microspheres to measure perfusion: validation of a neutron activation assay technique. *Am J Physiol Heart Circ Physiol*;280:H108-16.
- [4] Bland JM and Altman DG (1986). Statistical methods for assessing agreement between two methods of clinical measurements. *Lancet* 1:307-310.